


# TURBICUBE 20

**Turbidity transmitter**  
**From 0.01 to 20 FNU**

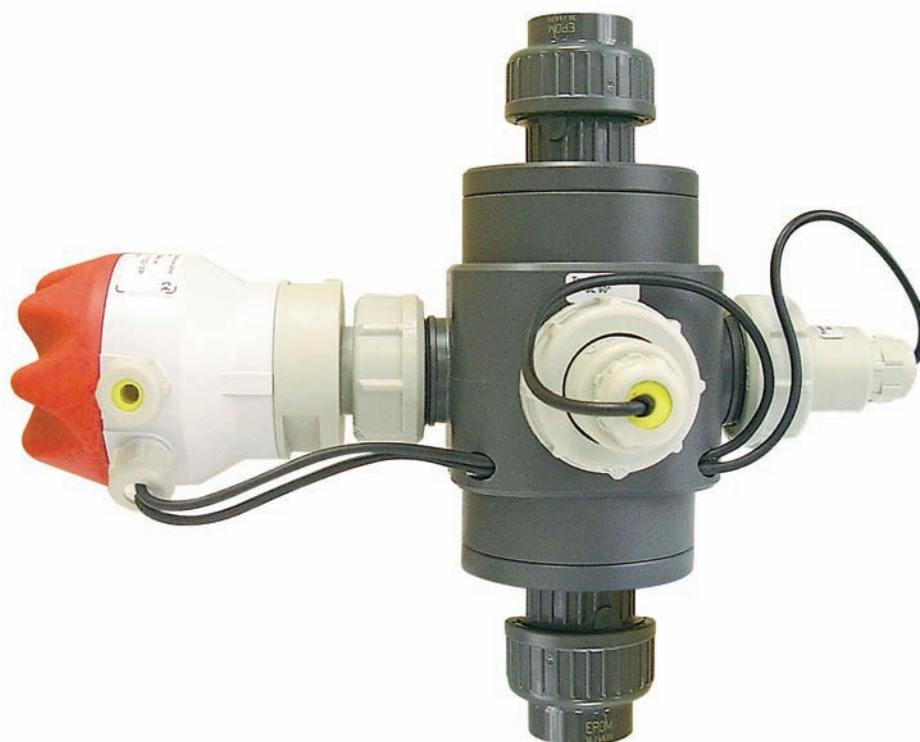

## INSTRUCTION MANUAL

**BAMO MESURES**

22, Rue de la Voie des Bans - Z.I. de la Gare - 95100 ARGENTEUIL

Tél : (+33) 01 30 25 83 20 - Web : [www.bamo.fr](http://www.bamo.fr)

Fax : (+33) 01 34 10 16 05 - E-mail : [info@bamo.fr](mailto:info@bamo.fr)

Turbidity transmitter  
**TURBICUBE 20**

16-04-2009

444 M1 01 D

**MES**

**444-01/1**

## SAFETY PRECAUTIONS

Only qualified person should operate, install and assure the maintenance.  
All International and European recommendations on electrical installation should be applied.

- The device may only be connected to supply power, which complies with the specifications included in the technical data!
- The device must be disconnected from all sources of power during installation and maintenance work!
- The device may only be operated under the conditions specified in the operating instructions!

## FUNCTIONS - DESCRIPTION


The turbidity-measuring device determines the turbidity of liquids using the light absorption and scattered light measuring method. The inline measuring cell at the sensor set makes use of two IR transmitters and one IR receiver in pulsating light mode (IR measuring method according to ISO 7027). The interconnected BAMOPHOX TUR measuring amplifier (option) analyses the 4 to 20 mA signal generated by the sensor set.

## MOUNTING

- The fixture must be installed **vertically!** – Best installation is the mounting in an ascending tube with slow down section 600 mm in front and 400 mm behind the turbidity-measuring device.
- The sensor fixture must be completely filled with liquid during the performance of measurements.  
Install to the vertical portion of a siphon trap if necessary.
- Air bubbles distort measurement results.
- Glass windows must be clean – clean them at regular intervals as required.

## SET UP – DISPLAYS

The sensor set consists of a receiver module with microprocessor-controlled analysis electronics and two emitter modules. The sensor set generates a 4 to 20 mA output signal in accordance with the following diagram. Measuring ranges are selected with the help of the DIP switches on the receiver module.

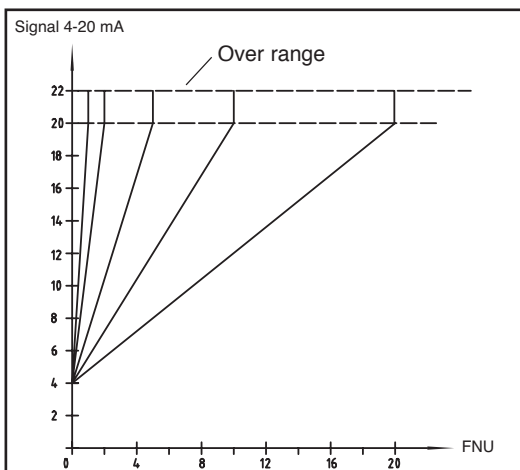


**Note:** The turbidity measuring instruments are calibrated with the internationally specified standard suspension Formazin.

The indication takes place thus not in form of the measured light intensity, but as concentration of the Formazin calibration suspension.

During the measurement with any liquid, this means thus that the liquid concerned causes the same light scattering as the standard suspension of the indicated concentration.

Measured values of other turbidity measuring instruments, which use other calibration suspensions and measuring angle, cannot be compared directly with those with Formazin calibrated measuring instruments.

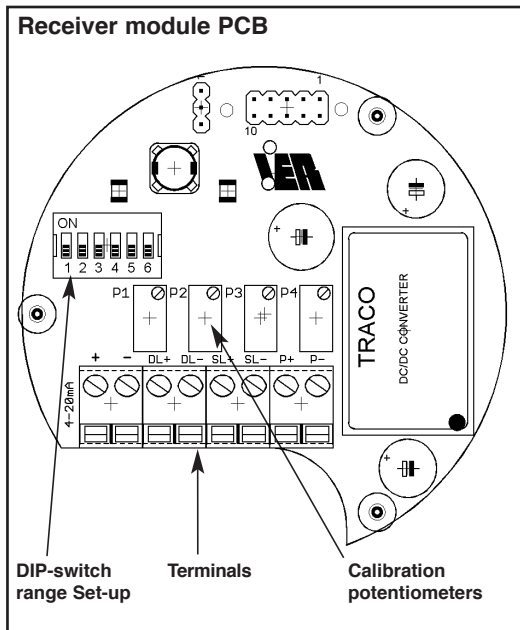

Measuring range	DIP1	DIP2	DIP3	DIP4	DIP5	DIP6*
MB1 = 0,01... 1 FNU	ON	ON	OFF	OFF	OFF	OFF
MB2 = 0,01... 2 FNU	OFF	OFF	ON	OFF	OFF	OFF
MB3 = 0,01... 5 FNU	ON	OFF	ON	OFF	OFF	OFF
MB4 = 0,01...10 FNU	OFF	ON	ON	OFF	OFF	OFF
MB5 = 0,01...20 FNU	ON	ON	ON	OFF	OFF	OFF

\*) **DIP6** / ON = Colour fouling compensation is switched on.  
(function only valid for DN 20 to DN 65)

	Indication
Green LED = 1Hz blinking	Ready, measuring in operation
Green LED = permanent ON	Ready, measuring not in operation
Green LED = OFF	No power supply, or defective

	Fault indication
Red LED = ON	Measuring circuit faulty, (short circuit, or broken) (cort circuit ou rupture)
Red LED = 1Hz blinking	Glass dirty or too much colored (damping factor > 20 dB)

**Signal in limit conditions:**


- 0 mA = wrong connected and / or dip-switches wrong adjusted
- 4 mA = 0 FNU (clearest water, pipe filled)
- 20 mA = 100% output acc. to adjusted range (pipe filled)
- 22 mA = over range
- 21 mA = general failure on electronics

**When pipe is empty:**

- if there are no water drops on the glasses the output will be a little bit higher than 4 mA (depending on the refraction index of air-molecules).
- if there are water drops on the glasses the output is higher than 4 mA, but the signal depends on size and quantity of water drops.

**So it's important to install the turbidity measurement system always in such a way that the pipe is filled at any time (vertically or with a siphon). That's valid not only for TURBICUBE but for all systems on the market.**

**WIRING**

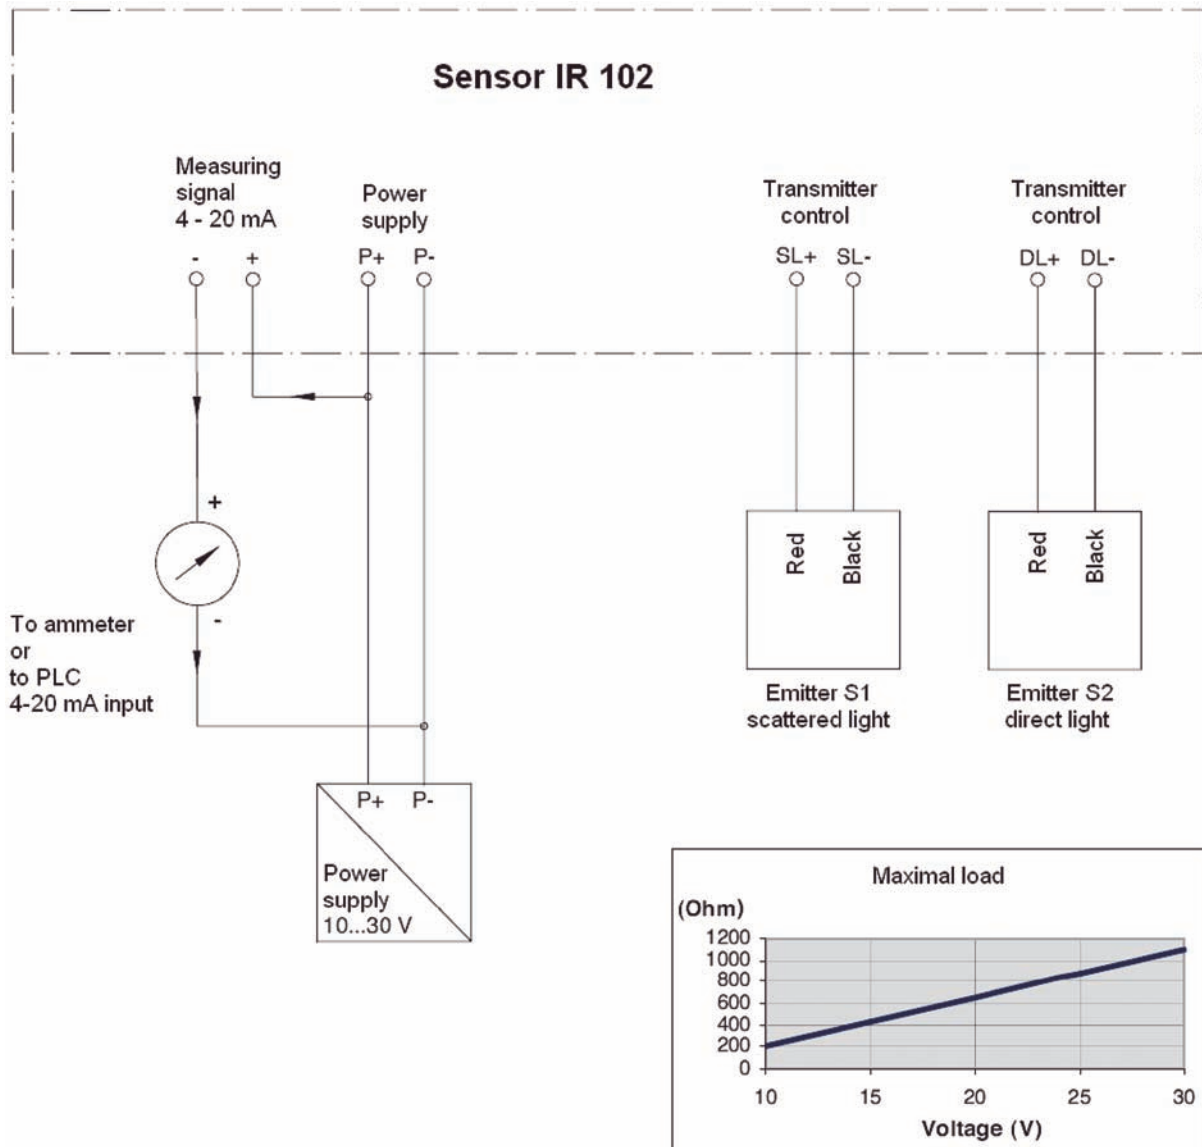

**NOTE:**

The measuring output "4-20 mA" is a current drain, this means, the output channel has the same electrical behaviour as a variable resistor.  
An active power supply for the measuring circuit is always needed.

For connection to BAMOPHOX TUR, please see specific documentation msa436-01.

## MAINTENANCE


Cleaning intervals depend upon the type of liquid medium and must be determined by the user.

### Cleaning the lenses:

- Disconnect the turbidity-measuring instrument from all sources of power.
- Depressurize pipes and empty liquid medium from the device.
- Remove the transmitters and the receiver from the fixture by unscrewing the sleeve nuts.



1) Screw the ETR-glass with the included tool and remove.

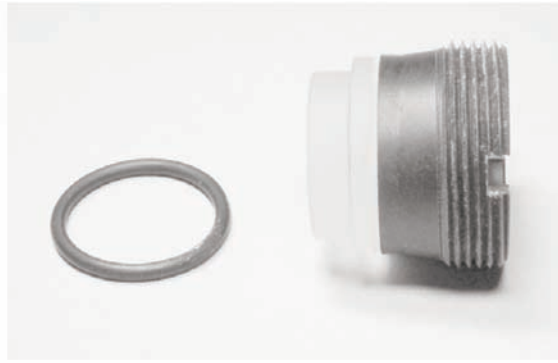

2) Clean the lens – **Do not use abrasive cleaners, which may cause scratching!!**

### Mounting:

- **Note: Inspect the O-ring before reassembly and replace if necessary.**
- Tighten the ETR-glasses with the included tool.
- Before reinstalling the transmitters and the receiver, refill the fixture with liquid medium and inspect for possible leaks.



Observe positioning of hole and pin!



### Note for cold fluids:

- The fixture has to be installed to the pipeline with mounted sensors only.
- For cleaning the glasses, dismantle the complete fixture, after cleaning install as described above

# CALIBRATION

## Factory Calibration

The sensor set is equipped with a calibration constant as a design feature.  
As a rule, no recalibration is required.  
Calibration point accuracy is better than 2%, and drift is less than 1% per year.



## Test Equipment Monitoring

If device calibration testing is required as part of the respective quality assurance system for test equipment monitoring, calibration can be checked with the calibration rods, and the device can be readjusted if necessary. A suitable calibration standard is delivered with each turbidity-measuring instrument. Each calibration standard is matched to the specific circumstances of the mating turbidity-measuring instrument and cannot be used for other measuring instruments of the same type!


**The calibration standard and the turbidity-measuring instrument must have the same serial number!**

## Caution:

**It must be assured that all utilised control and switching devices are switched off during recalibration!**

## The following adjustment sequence must be adhered to!

1. Clean all lenses and wipe them dry (all visible water droplets and water film must be removed!).
2. Then reinstall the lenses for the receiver and the S1 transmitter only.  
Do not yet install the lens and the compression disc for the S2 transmitter (180° scattered light)
3. Reinstall the S1 transmitter and the receiver.
4. Remove the KN 20 calibration rod from the box.
5. Insert the calibration rod into the fixture
6. Mount the S2 transmitter to the calibration rod (observe the locking pin)

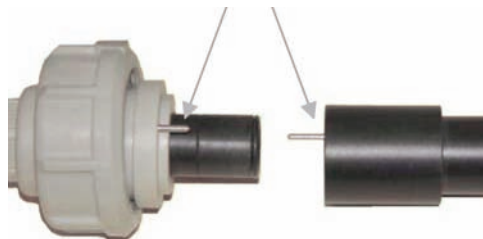

7. Insert the calibration rod with attached transmitter completely into the fixture (observe the locking pin), and tighten the sleeve nut.
8. Set the DIP switches to the MB5 range = 0.01 to 20FNU (ON/ON/ON/OFF/OFF/OFF)
9. Switch supply power back on again – the status LED blinks!
10. Compare the set point value and the actual value.  
Set point 1 (SW1) = set point on the plate in the box of the KN20 calibration rod  
Actual value = measured value
11. Set point vs. actual value deviation:  
Less than  $\pm 5\%$ , measuring instrument is OK  
Greater than  $\pm 5\%$ , adjust actual value with potentiometer P4
12. Remove transmitter and calibration rod
13. Mount glass with sealing ring and compression disc and transmitter S2
14. Select the right DIP-switch setting for operation

## TECHNICAL FEATURES


Terminal housing:	PBT, IP65
Auxiliary power supply:	24 V DC (10...30 V DC); connected load 0.5 W. Note: connecting also the measuring circuit to the auxiliary power supply of the load, it increases of 24 V DC x 20 mA = 0,48W
Power consumption:	0,6 W
Output signal:	4-20 mA for connection to the BAMOPHOX TUR 436. Note: if a different measuring amplifier is used, an external 10 to 30 V DC voltage source is required.
Ambient temperature:	+ 5...+ 45°C
Process temperature:	+ 5...+ 60°C
Accuracy:	± 5% reading, ± 1% full scale in use
Maximum pressure:	6 bar at 20°C / 1 bar at 60°C
Status indication:	correct is a green LED; failure is a red LED
Selectable ranges:	from 0,01 to 1 / ...2 / ...5 / ...10 / ...20 FNU
Wetted parts:	Plane wall measuring cell from polymers (PCV or PP) and anti-fouling ETR-glasses.
Sealing:	EPDM (FPM as an option)
Process connections:	from DN 20 to DN 100, flanges or union socket ends
<b>CE Mark:</b>	In accordance with low-voltage directive (73/23/EWG), EMC directives (89/336/EEC)

## DIMENSIONS

DN	(d)	PVC model		ppH model	
		L (-0/+2 mm) (Union socket ends)	L (±2 mm) (Flanges acc. DIN 2501)	L (-0/+2 mm) (Union socket ends)	L (±2 mm) (Flanges acc. DIN 2501)
DN 20	Ø 25	240	240	300	300
DN 25	Ø 32	240	240	300	300
DN 32	Ø 40	240	240	300	300
DN 40	Ø 50	240	240	300	300
DN 50	Ø 63	262	262	342	300
DN 65	Ø 75	314	314	342	300
DN 80	Ø 90	347	347	394	400
DN 100	Ø 110	347	347	394	400

**Caution:** Only for vertical ascending tubes!

Mounting in a ascending tube with slow down section in front and behind the TURBICUBE is optimal.

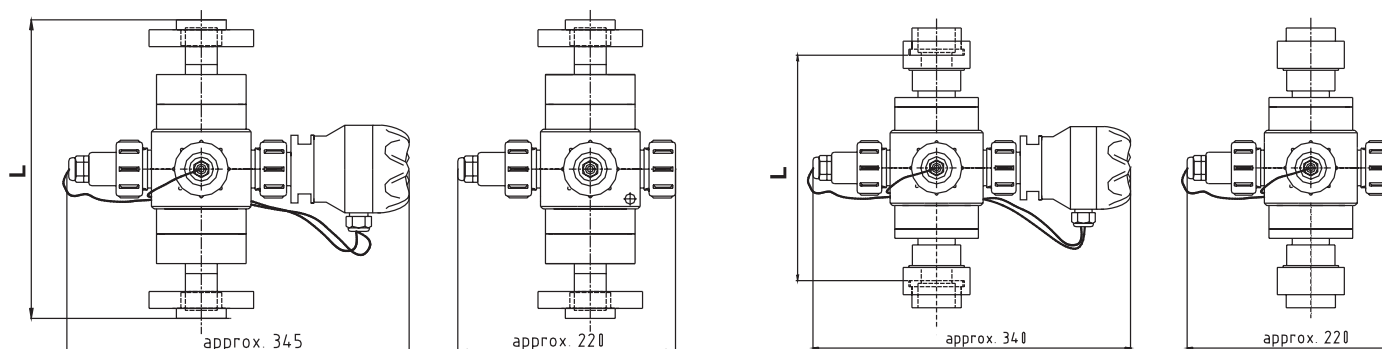

**Example: Turbicube FF ..2**  
ppH model with flanges acc. ISO 7005,  
EN 1092, DIN 2501

**Example: Turbicube VV ..2**  
PVC model with union socket ends